
MINICAP *FLEX-PIERCING*

MULTI-ASSAY SOLUTION
FOR AUTOMATED
ELECTROPHORESIS

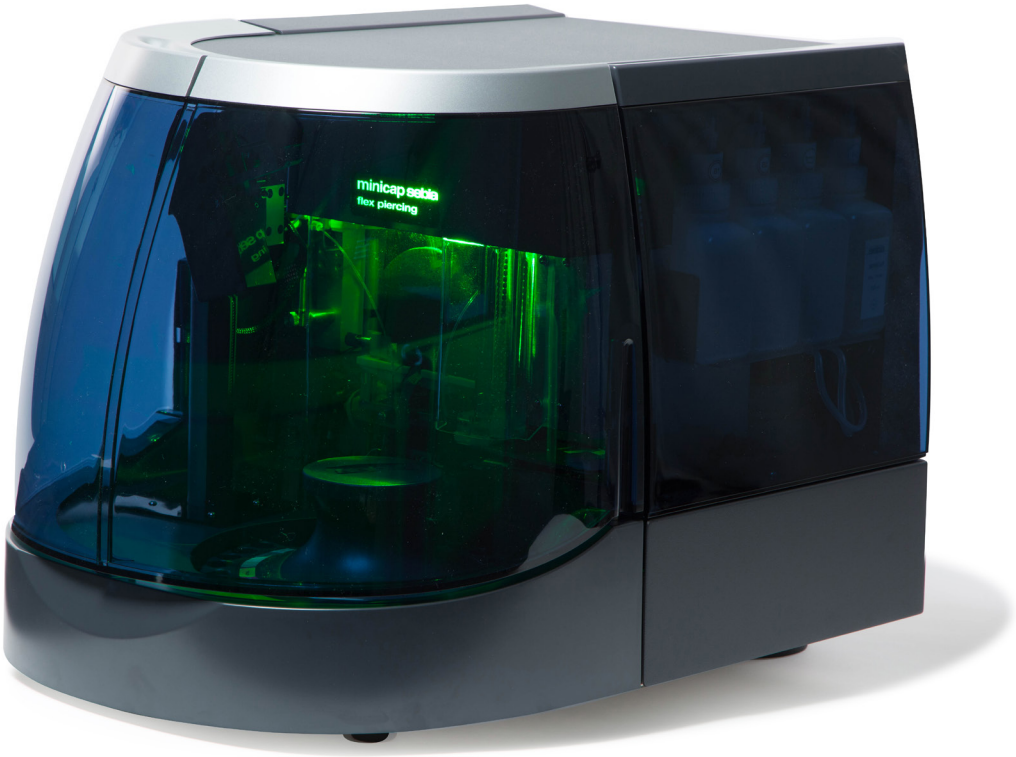

sebia


The new language of life

Multi-assay instrument
Extended test menu


- Serum Protein Electrophoresis (SPE)
- Serum Immunotyping
- Hb A1c
- Hemoglobin Electrophoresis
- CDT/CDT_{IFCC}

Capillary Electrophoresis
Analytical performance


- Fast protein separation
- Excellent resolution and reproducibility

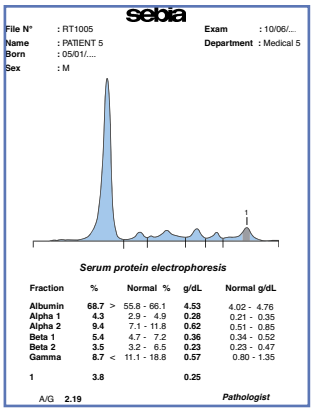


PROTEIN(E) 6

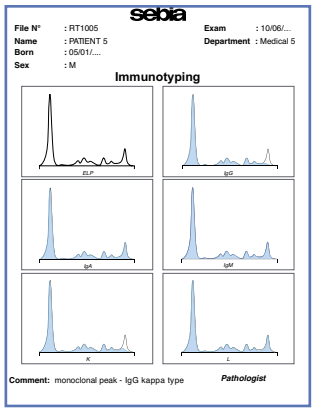


IMMUNOTYPING

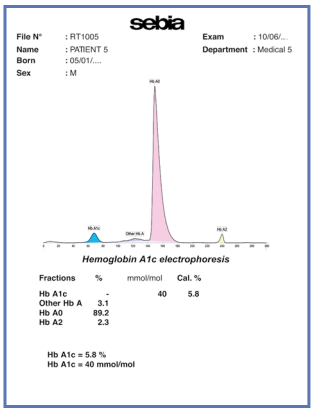

HbA1c

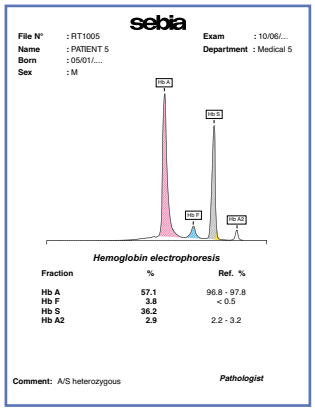

HEMOGLOBIN(E)

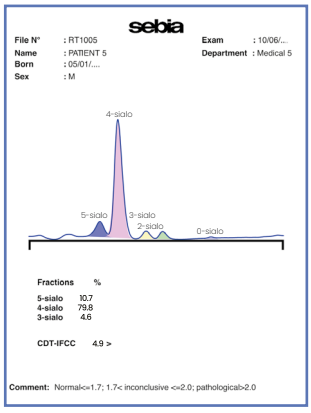

CDT, CDT_{IFCC}

Sample processing
Fully automated

- Sample mixing and cap piercing capabilities with whole blood technics
- Full traceability from primary tube to final result

IT integration
Efficient information flow

- Networking of all Sebia instruments
- Remote validation of the results
- Off-site remote access
- Unlimited data storage


PHORESIS

Interpretation software
and results validation

- Intuitive and user-friendly interface
- Multicriteria search function
- Automatic recall of patient's history
- Automatic triage of the results

Performance
High throughput

- SPE: 18 tests/h
- Hb A1c: 8 tests/h
- Hemoglobin: 7 tests/h
- CDT & CDT_{IFCC}: 10 tests/h

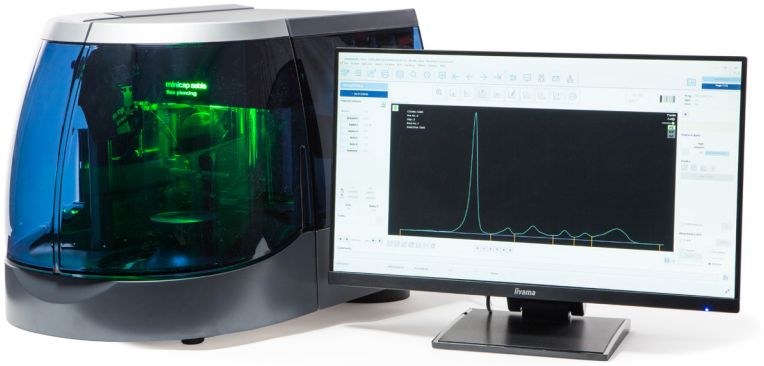

Specifications

- Reduced footprint
- Maximum sample loading capacity of 28 samples

Ordering *information*

Instruments

- MINICAP FLEX-PERCING 1232

Reagents

- MINICAP PROTEIN(E) 6 2203
- MINICAP HEMOGLOBIN(E) 2207
- MINICAP CDT 2208
- MINICAP Hb A1c 2215
- MINICAP IMMUNOTYPING 2300

Accessories

- BARCODES READER
  CAPILLARYS / MINICAP 1079

Consumables

- MINICAP FLEX-PIERCING
  CAPICLEAN 2251
- MINICAP
  REAGENT CUPS / 125 (3) 2281
- MINICAP
  LIDS FOR USED CUPS BINS (12) 2286
- CLEAN PROTECT 2059

Scan here
for more information on
MINICAP FLEX-PIERCING

For further information, please find your Sebia local representative to contact on our Website **www.sebia.com/sebia/worldwide-presence/**.

CE

Sebia | RCS Evry 672 041 902 | Parc technologique Léonard de Vinci | 27, rue Léonard de Vinci | CP 8010 Lisses | 91008 Evry cedex | France | Tel.: +33 1 69 89 80 80 | E-mail: sebia@sebia.com | **www.sebia.com**

©2025 **Sebia** - RCS Evry 672 041 902 | Parc technologique Léonard de Vinci | 27, rue Léonard de Vinci | CP 8010 Lisses | 91008 Evry cedex | France - Ref.: MFPB1EN - 03/2023
Non-contractual illustration - Sebia reserves the right to modify at any time and without notice the information contained in this document intended for healthcare professionals. This document contains information intended for wide distribution and may therefore contain product details or information that is not available or valid in your country. Carefully read the instructions in the reagent package inserts and instrument manuals.